

Electronic Supplementary Data

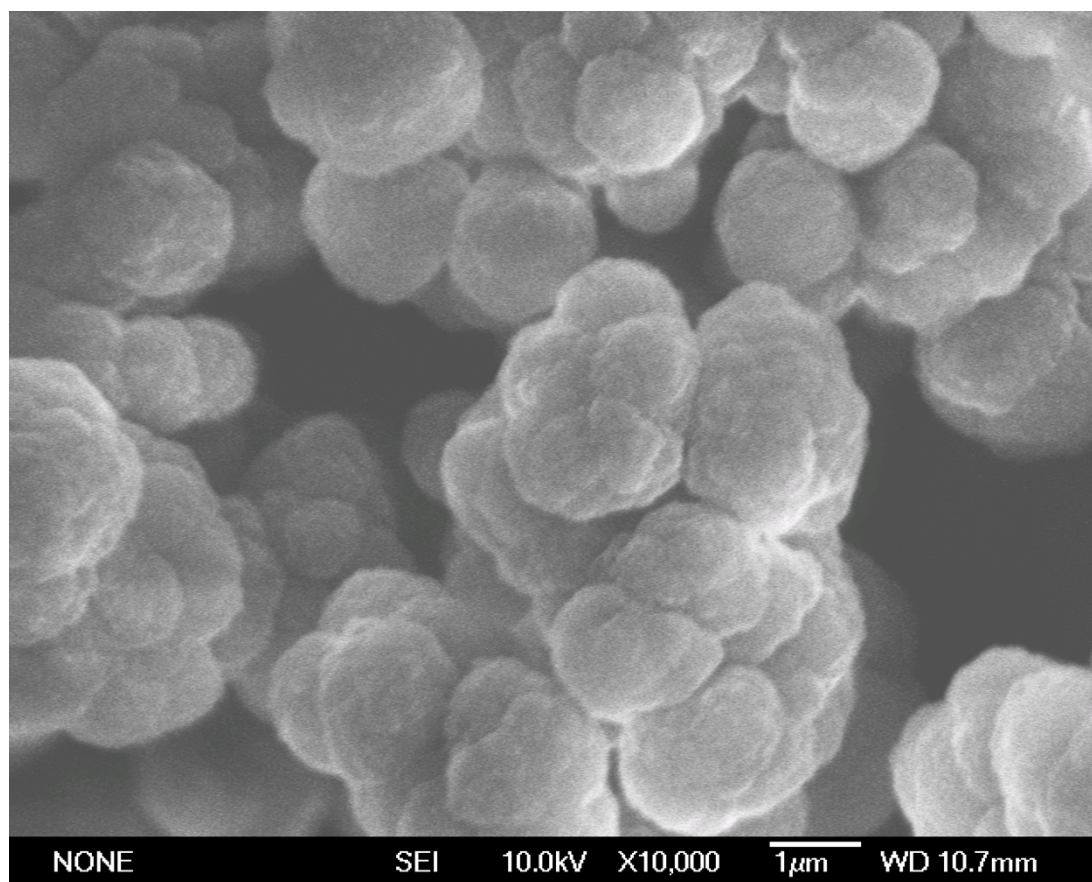


Figure S1

Experiment condition	Times
Sample flow rate	15
Sample pH	15
Effect of desorption solvent type	15
Eluent volume	15
Eluent flow rate	15
Sample volume	15
Salt effect	15
Stability of the column	15
Calibration curves	24
Repeatability	36
Recovery	36

Table S1