

Supplementary information

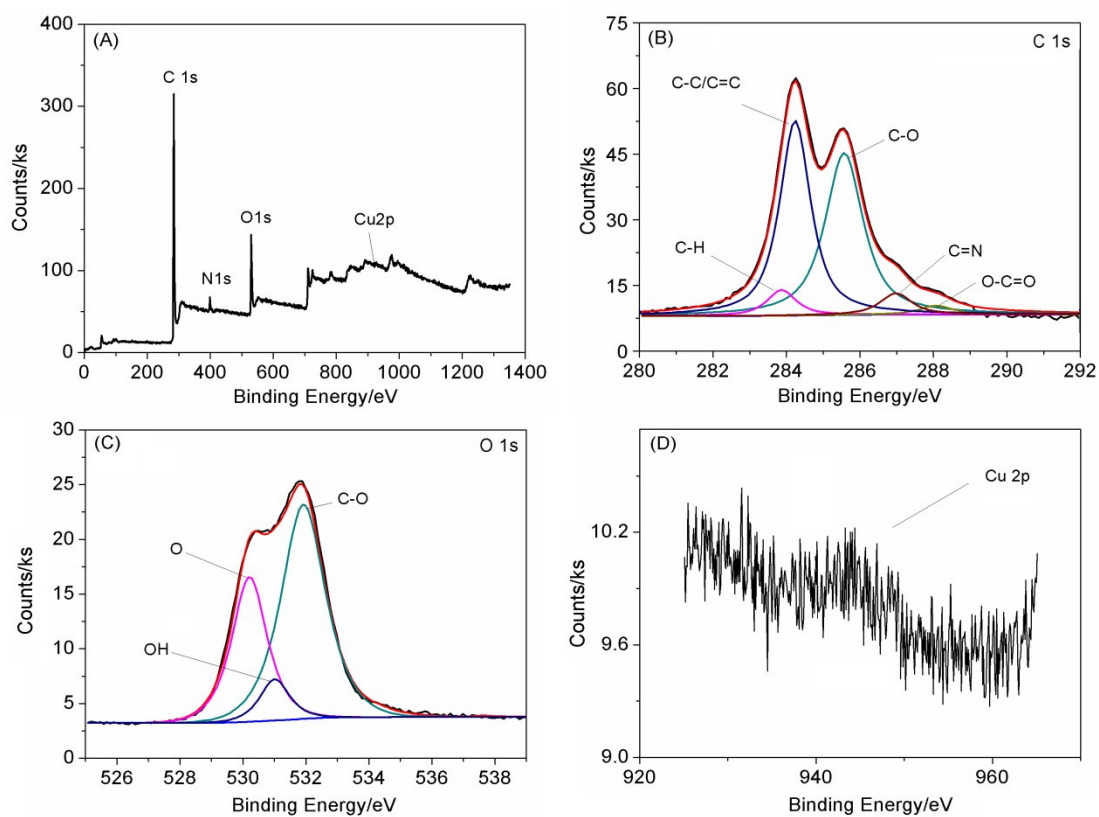


Fig. S1. XPS spectra of the Tyr-1-FP/rGO electrode: wide scan (A) and high resolution scans for C 1s (B), O 1s (C), Cu 2p (D).

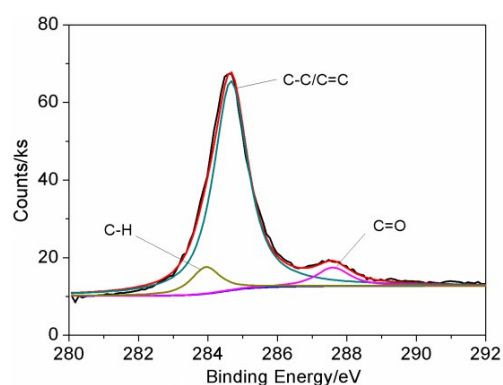


Fig. S2. XPS spectrum of the 1-FP/rGO: high resolution scans for C 1s.