

Supplementary Material

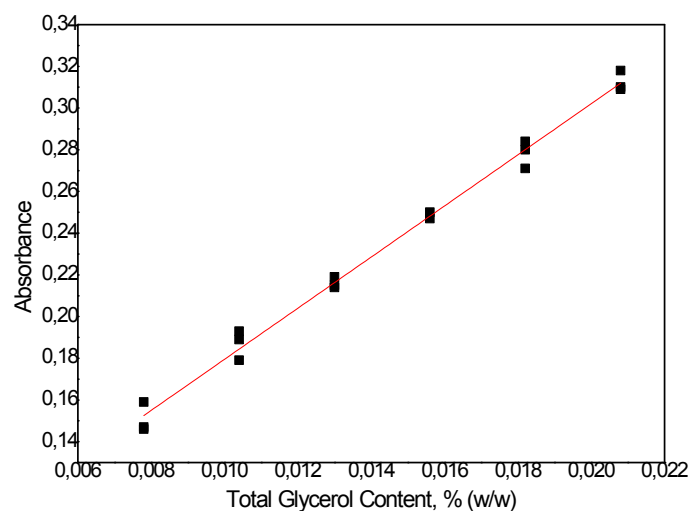


Fig. S1. Analytical curve obtained for glycerol standards in 4 mL of the commercial enzymatic kit ranging from 0.0078 to 0.0208% w/w.

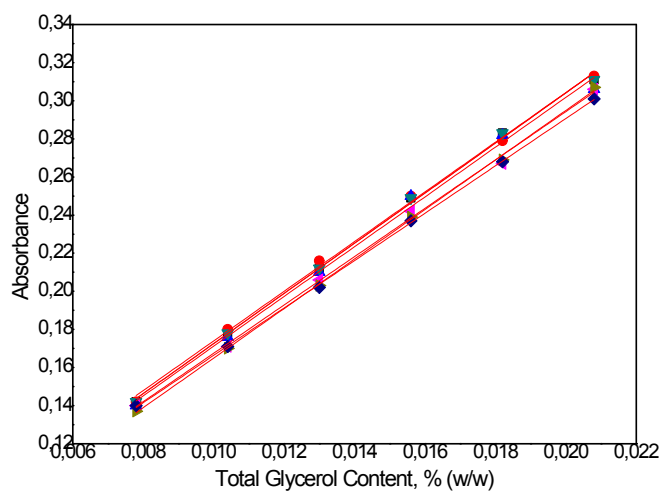


Fig. S2. Evaluation of the intermediate precision through several analytical curves plotted on different days, two lots of the enzymatic kit and different.