

Supplementary Material

Breast Cancer or Surrounding Normal Tissue? A Successful Discrimination by FTIR and Raman Microspectroscopies

Adriana P. Mamede^{a†}, Inês P. Santos^{a†*}, Ana L.M. Batista de Carvalho^a, Paulo Figueiredo^b, Maria C. Silva^c, Maria P.M. Marques^{a, d}, Luís A.E. Batista de Carvalho^a

^a "Unidade de I&D Química-Física Molecular" (QFM-UC) Department of Chemistry, University of Coimbra, Coimbra, Portugal

^b Pathology Department, Portuguese Institute of Oncology Francisco Gentil (IPOFG), Coimbra, Portugal

^c Surgery Department, Portuguese Institute of Oncology Francisco Gentil (IPOFG), Coimbra, Portugal

^d Department of Life Sciences, University of Coimbra, Coimbra, Portugal

[†]These authors contributed equally to this work

*Correspondence: ips@uc.pt

Table of Contents

Materials and Methods

Xylene ($C_6H_4(CH_3)_2$) and ethanol (99%) were purchased from Merck (Lisbon, Portugal).

Figures

Figure S1 – Home-made sample holders for the Raman WITec Alpha300R (A) and FTIR Bruker Hyperion 3000 (B) microscope tables, designed to ensure a location reproducibility of the measured regions of interest within the tissue, and the spatial complementarity between Raman and FTIR measurements.

Material and Methods

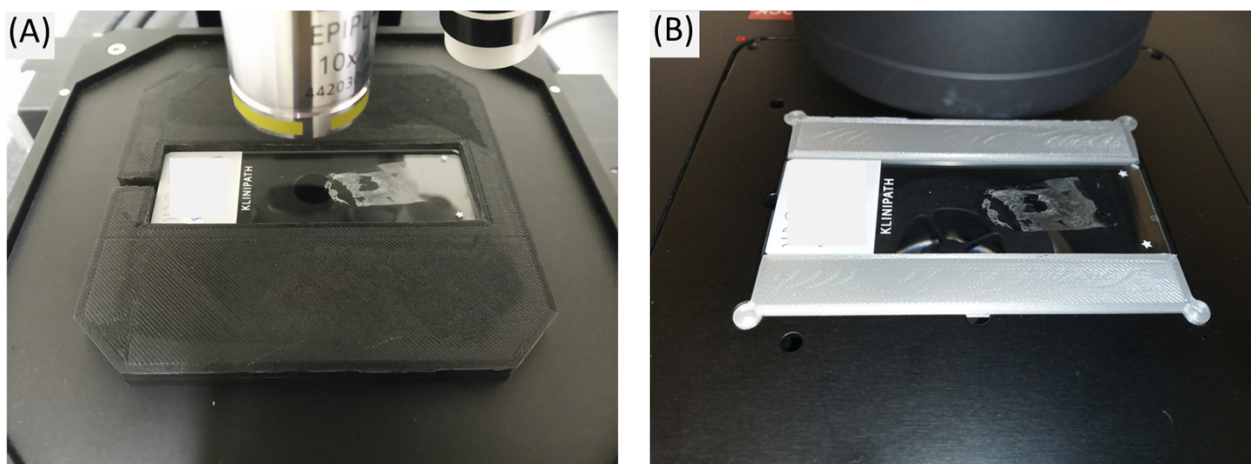


Figure S1. Home-made sample holders for the Raman WITec Alpha300R (A) and FTIR Bruker Hyperion 3000 (B) microscope tables, designed to ensure a location reproducibility of the measured regions of interest within the tissue, and the spatial complementarity between Raman and FTIR measurements.