

Figure S1. The schematic diagram of the online pre-column FRAP-HPLC screening system

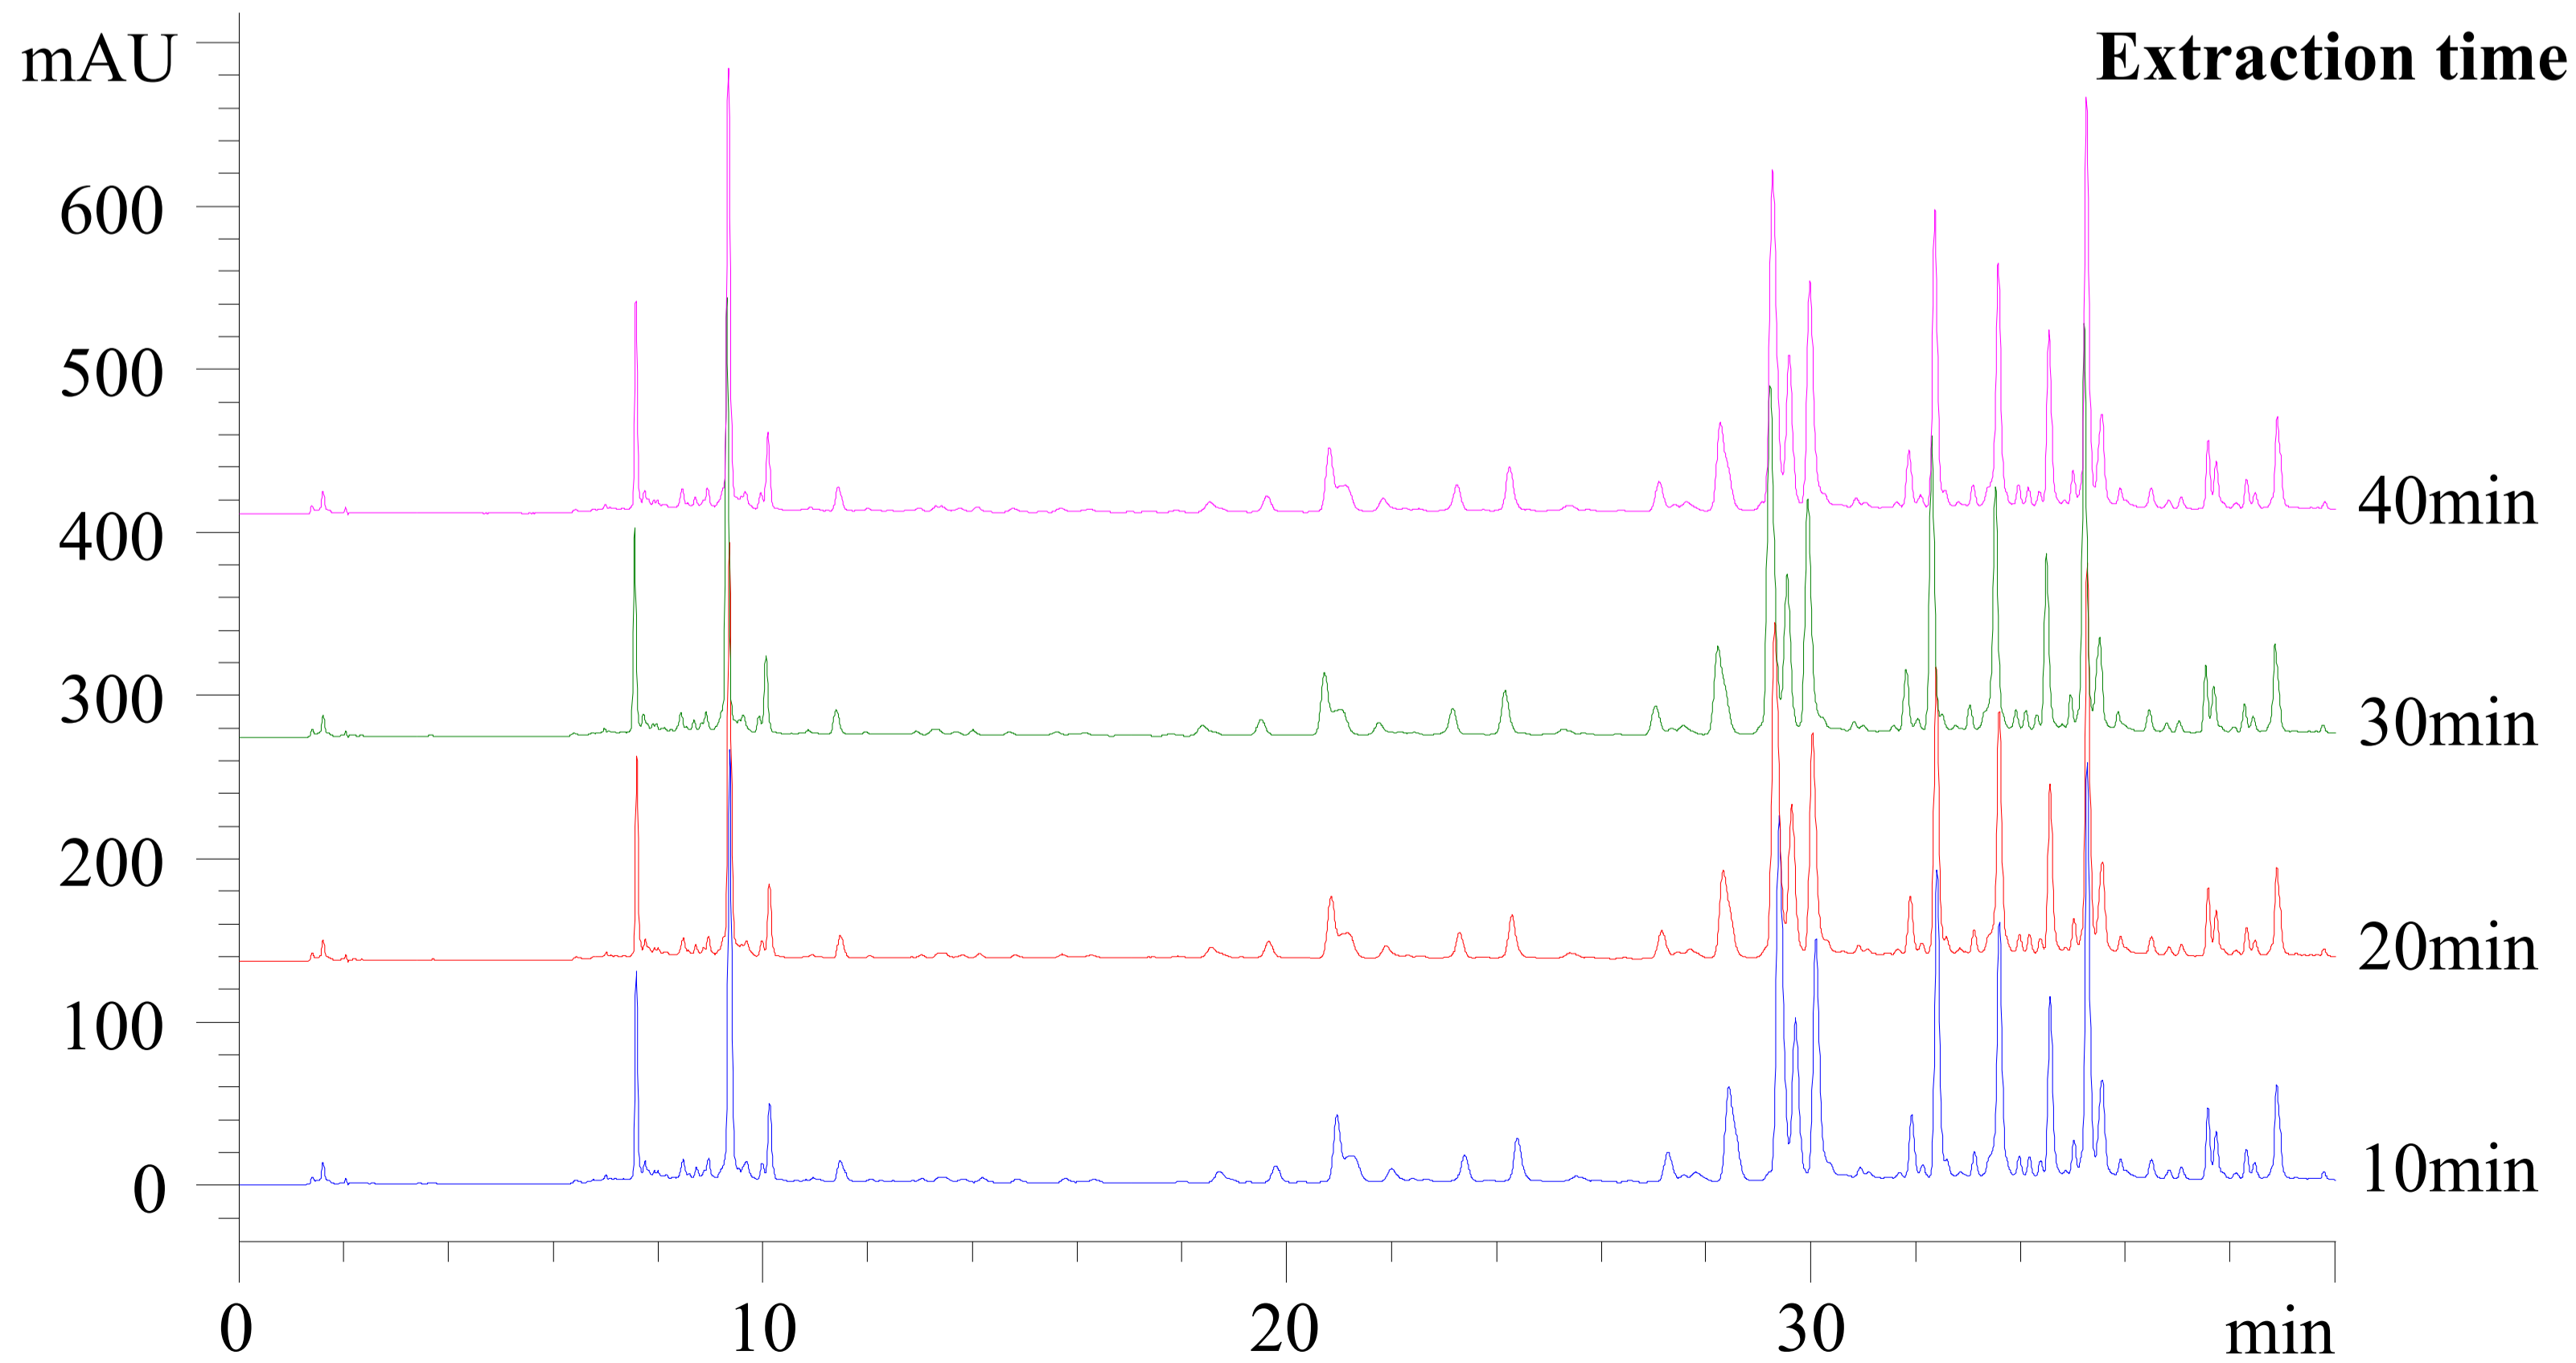
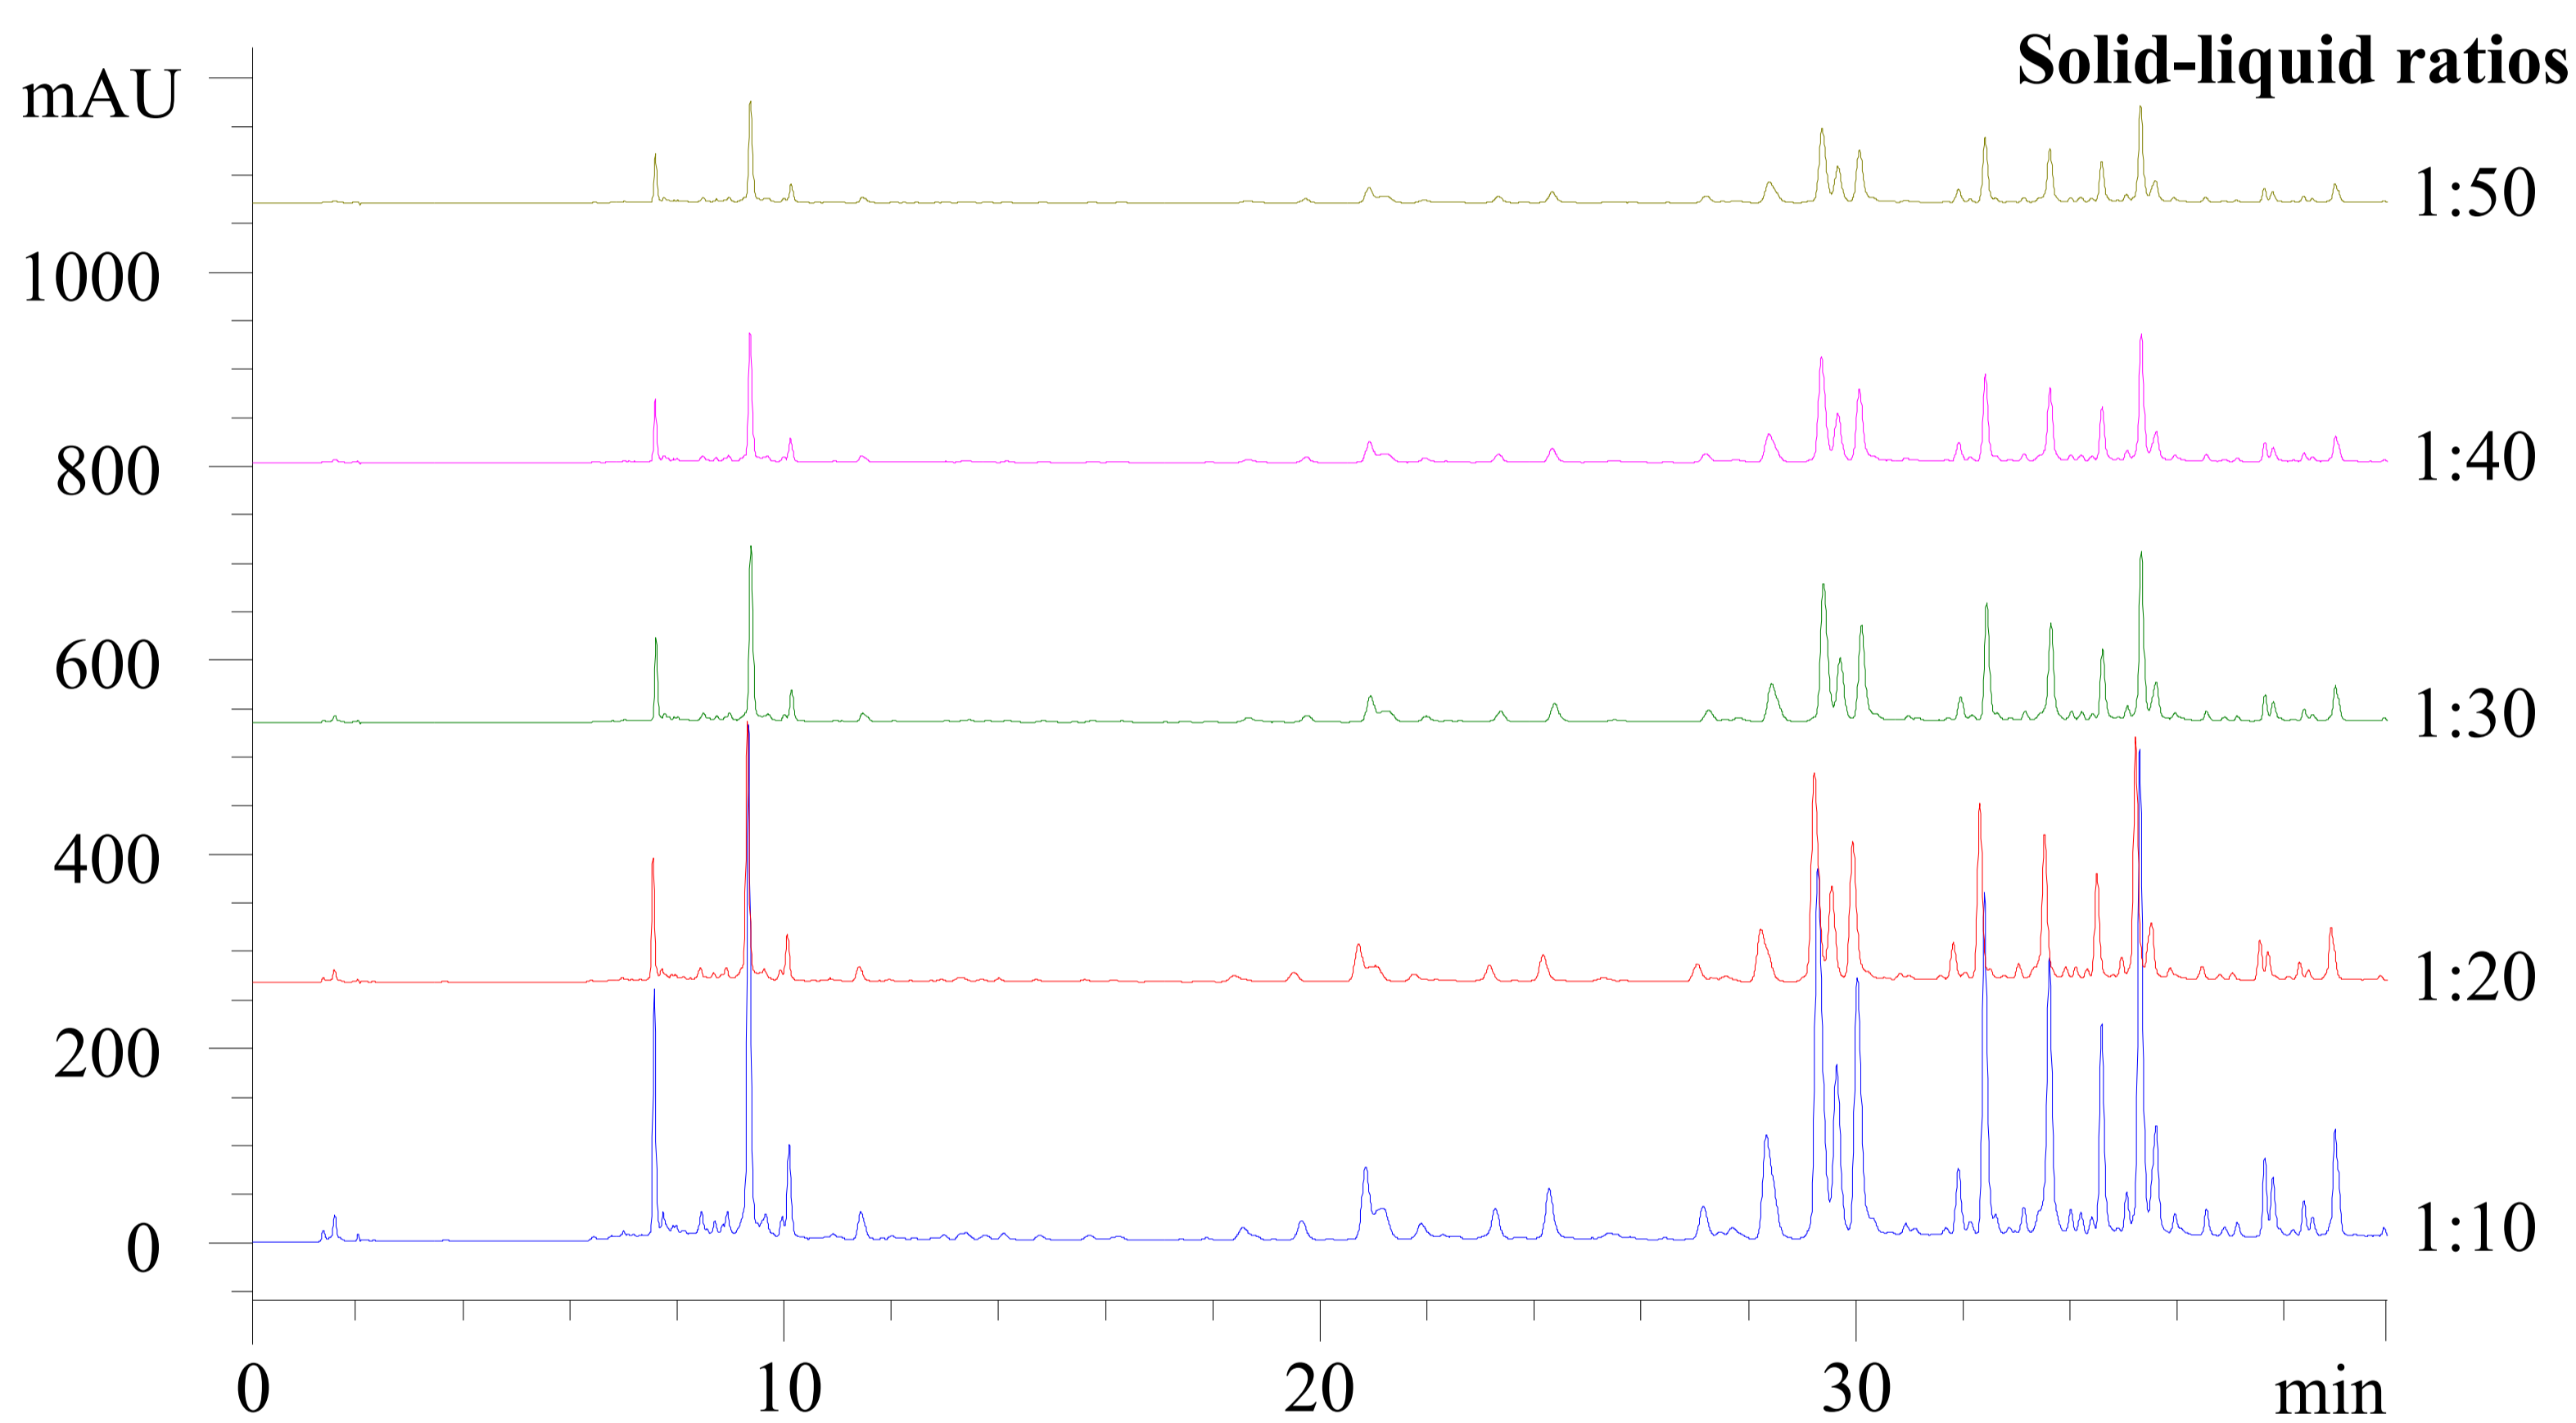
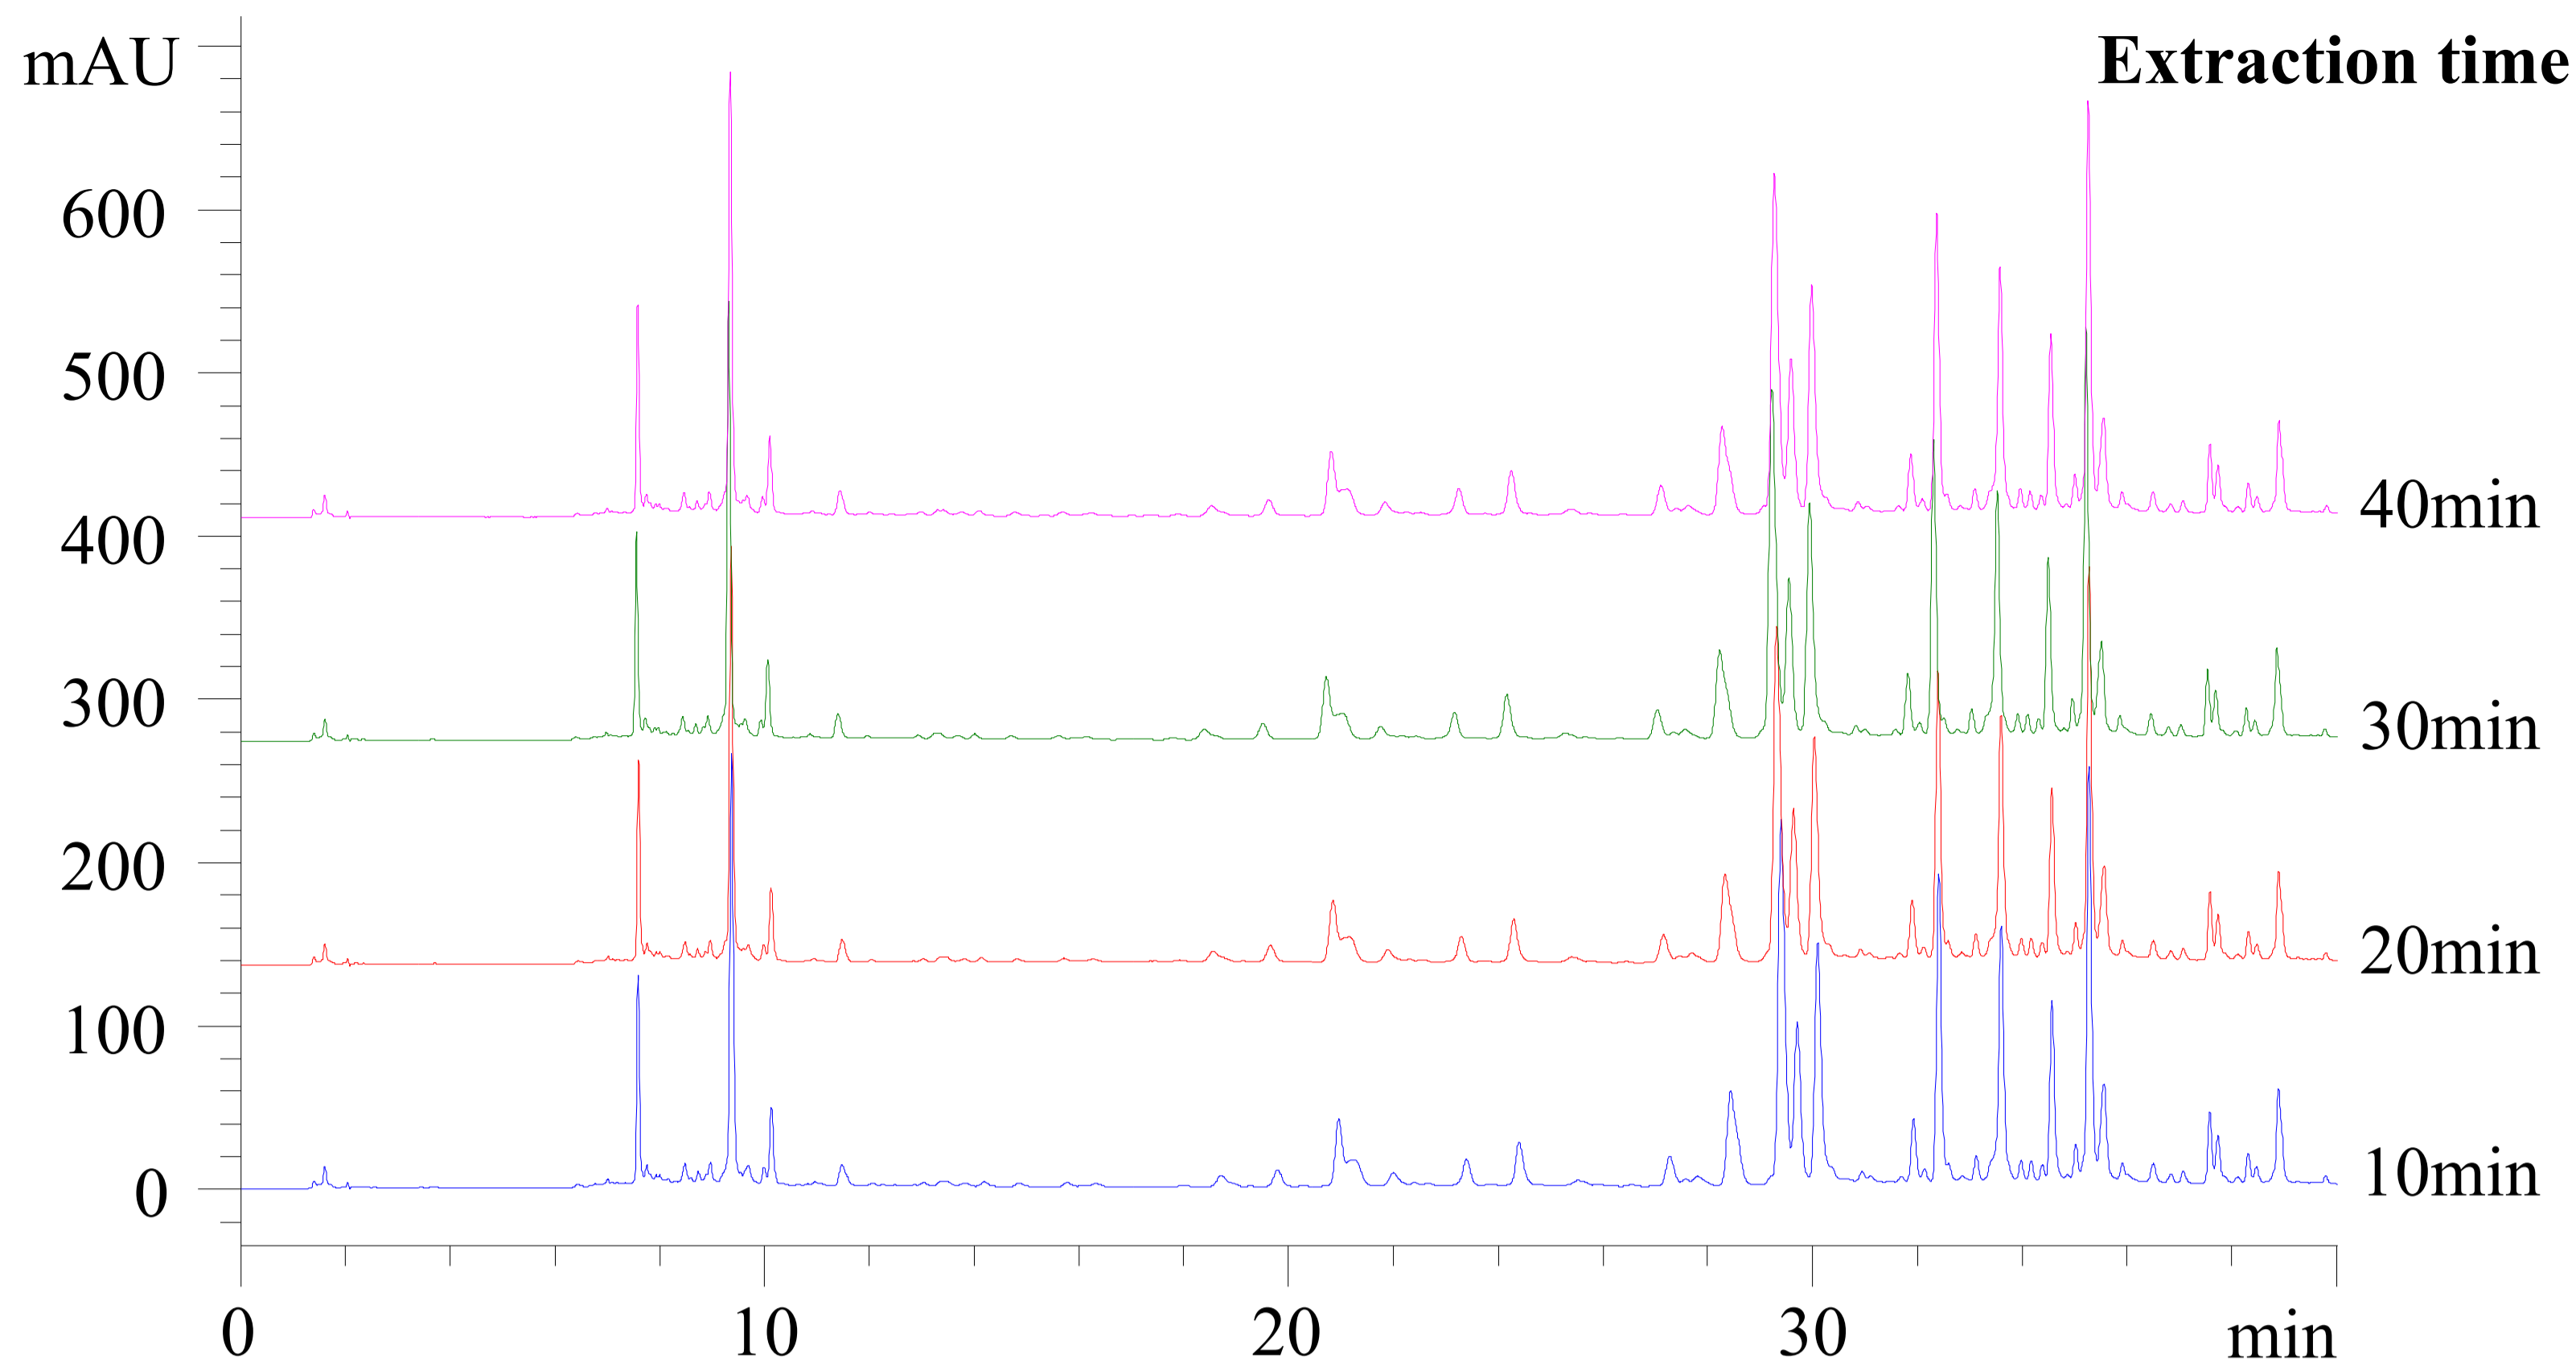


Figure S2. The results of UAE optimization

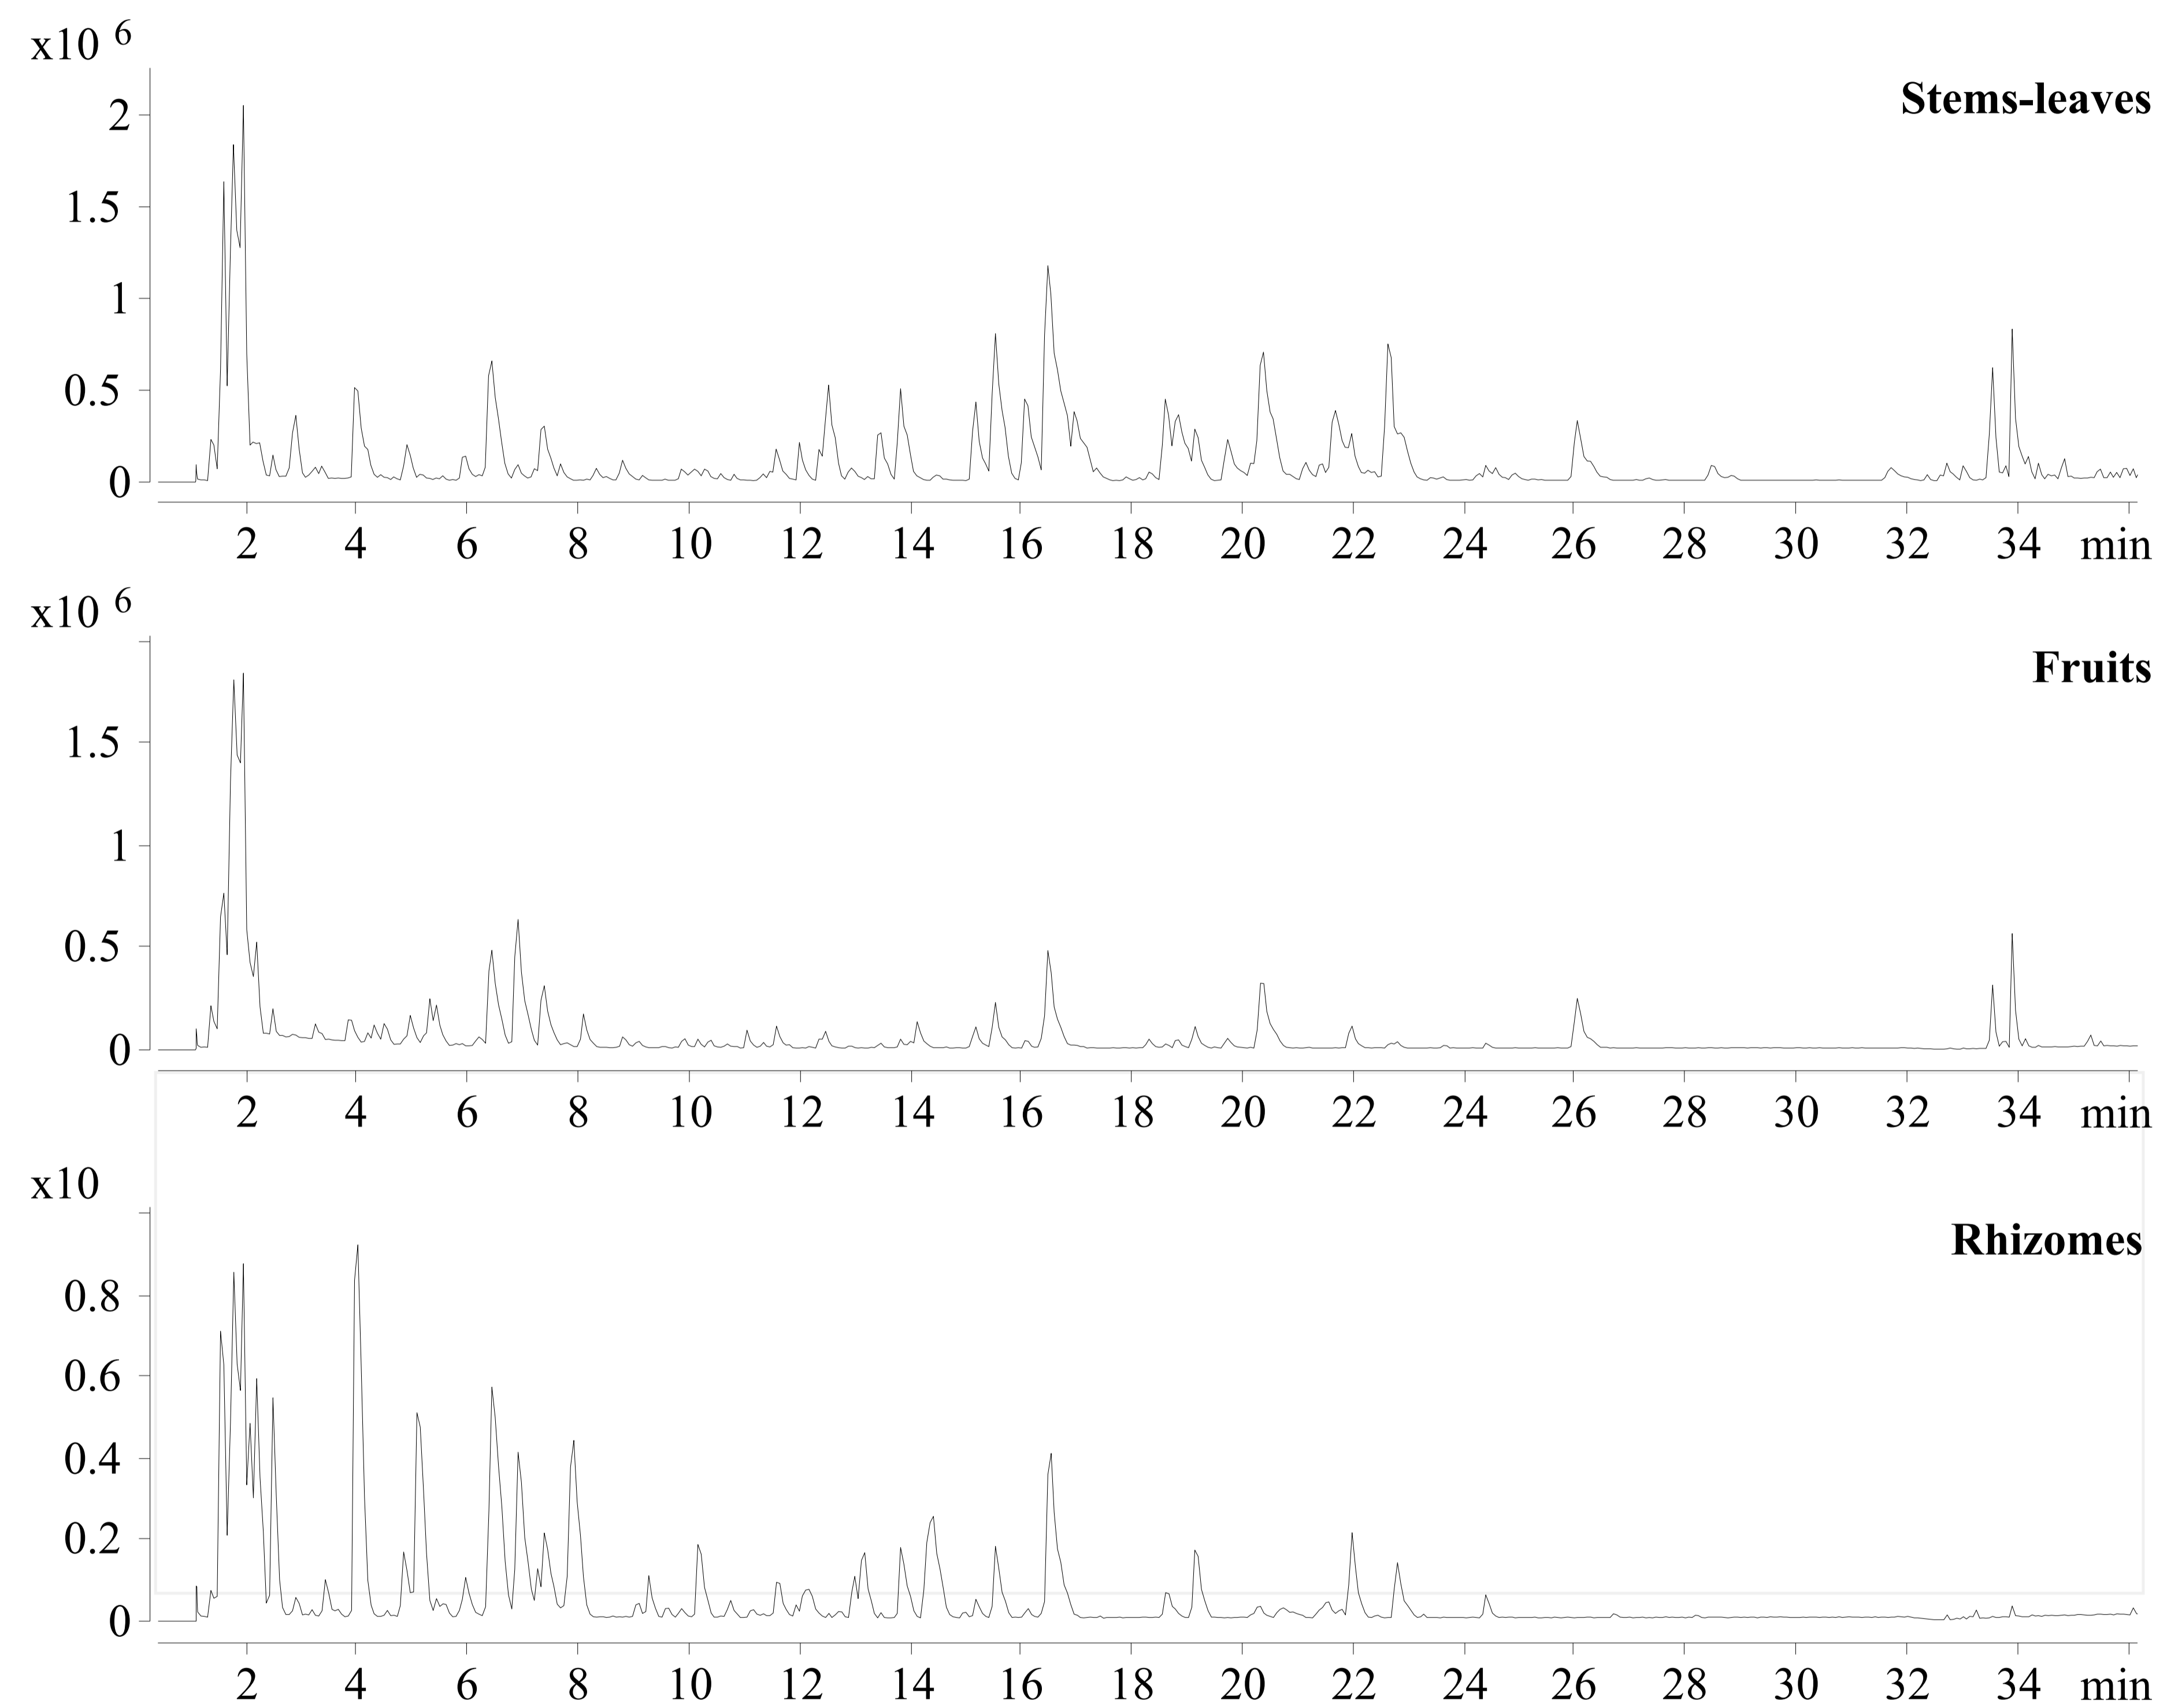


Figure S3. The base peak chromatograms of samples