



Supplementary Information 1: ^1H NMR spectrum of LaSOM 186 (Solvent: DMSO- d_6 . Equipment: Bruker Avance™ III spectrometer 400 MHz, Bruker Corporation, Billerica, Massachusetts, USA)

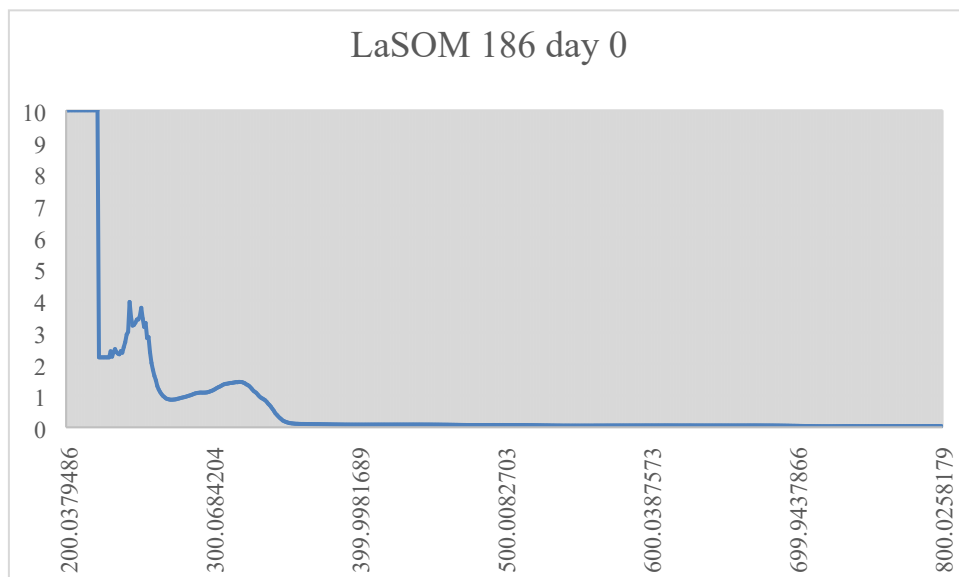

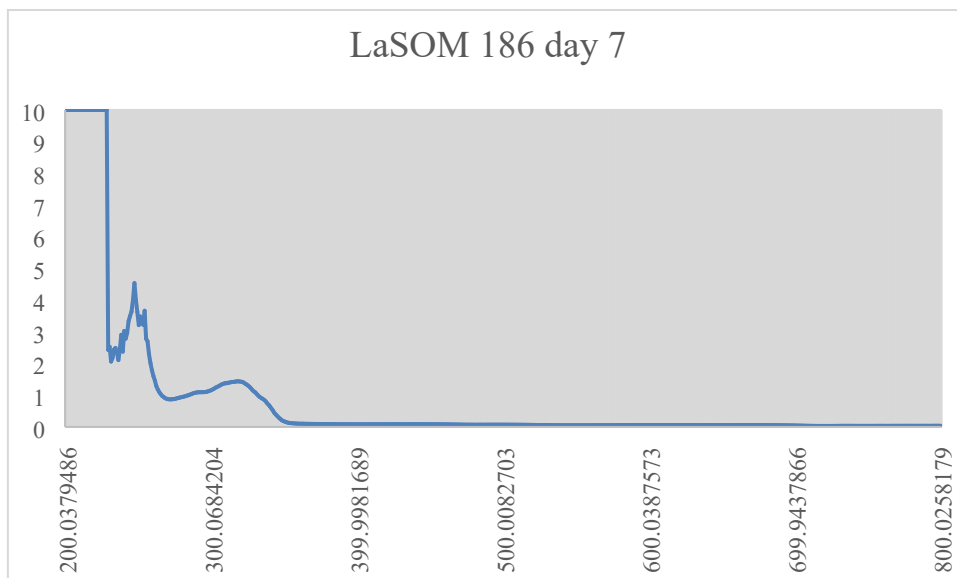

Supplementary Information 2: UV spectra of LaSOM 186 after 7 days (Solvent: DMSO. Equipment: Varian Cary® 50 UV-Vis Spectrophotometer, Agilent Technologies, Santa Clara, California, USA).