

Supplement

Advances in implants and bone graft types for lumbar spinal fusion surgery


Giles M. Cheers ^{1,*}, Lucas P. Weimer ¹, Carl Neuerburg ¹, Jörg Arnholdt ¹, Fabian Gilbert ¹, Christoph Thorwächter ¹, Boris M. Holzapfel ¹, Susanne Mayer-Wagner ¹, Markus Laubach ^{1,2,*}

¹ Department of Orthopaedics and Trauma Surgery, Musculoskeletal University Center Munich (MUM), LMU University Hospital, LMU Munich, Marchioninistraße 15, 81377 Munich, Germany

² Australian Research Council (ARC) Training Centre for Multiscale 3D Imaging, Modelling and Manufacturing (M3D Innovation), Queensland University of Technology, Brisbane, QLD 4000, Australia

* corresponding authors. Giles.Cheers@med.uni-muenchen.de, Markus.Laubach@med.uni-muenchen.de

Supplement 1. Representative image of an autologous bone dust collector.

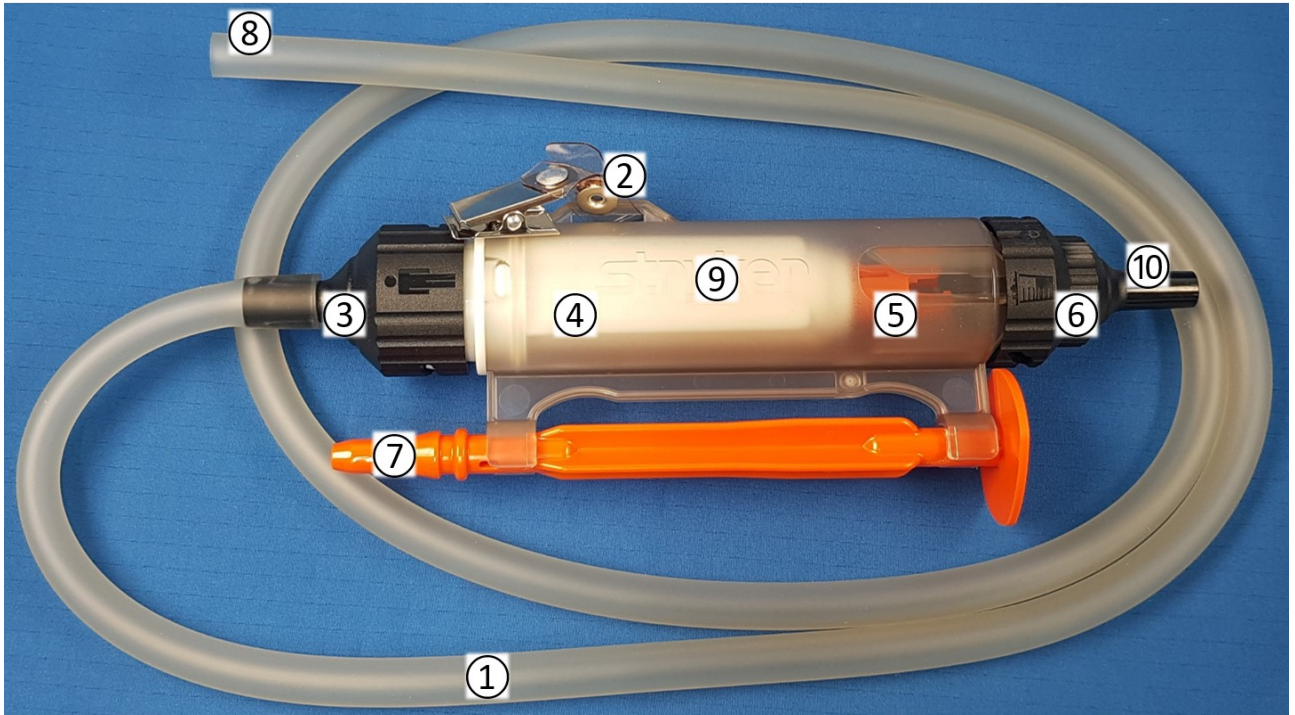

Key: 1 = inlet tubing, 2 = drape clip, 3 = inlet cap, 4 = device body, 5 = piston, 6 = outlet cap, 7 = plunger, 8 = inlet tube opening for connection to surgical suction tip, 9 = bone material filter, 10 = outlet site for connection to waste management system. Bone Vac was kindly provided by Stryker.