

Supporting information

A High-Performance Flexible Humidity Sensor based on TiO₂-MWCNTs Nanocomposite for Human Healthcare

Ankit Kumar^{1,3}, Parvesh Kumari^{1,3}, M. Senthil Kumar^{2,3}, Gaurav Gupta¹, D.D.
Shivagan^{1,3}, Komal Bapna^{1,3*}

¹ Temperature and Humidity Metrology, CSIR- National Physical Laboratory, Dr. K. S.
Krishnan Marg, New Delhi 110012

² Sensor Devices and Metrology, CSIR- National Physical Laboratory, Dr. K. S. Krishnan
Marg, New Delhi 110012

³ Academy of Scientific & Innovative Research (AcSIR), Ghaziabad-201002, India

*E-mail: komal.bapna@nplindia.org

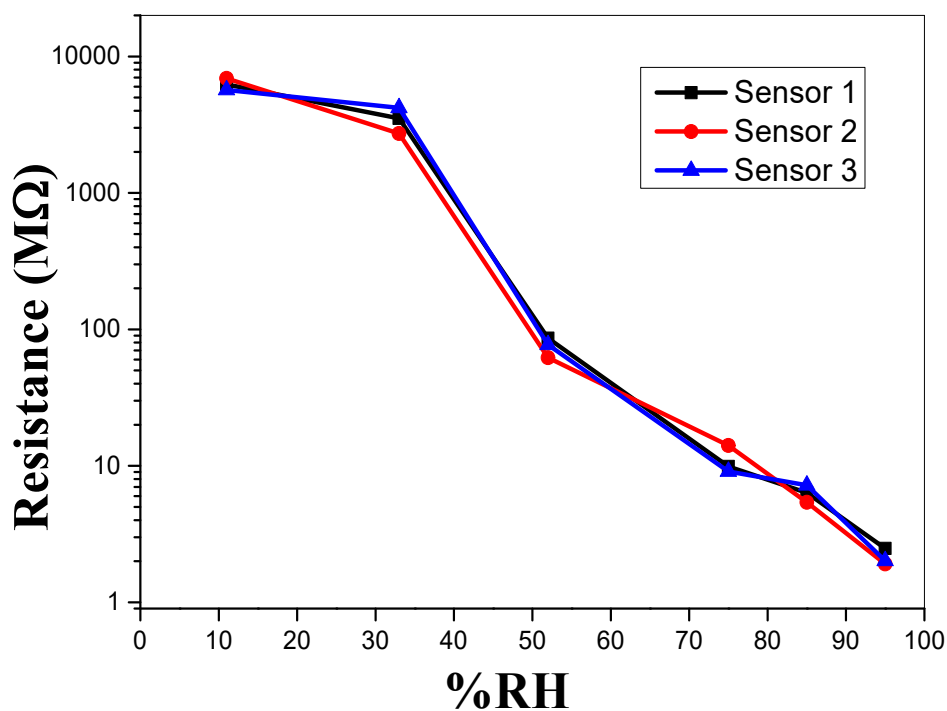


Fig. S1. The responses of the 3 composite sensors with respect to relative humidity.

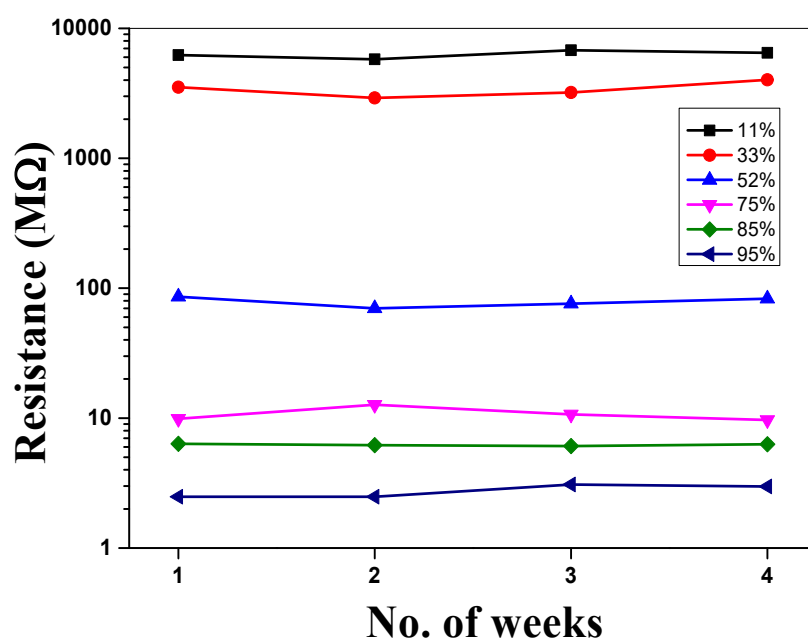


Fig. S2. Long term stability of the TiO₂-MWCNTs composite based sensor.