

Unilateral thermosensitive Janus hemostatic dressing for matching coagulation physiological processes

Chuanjuan Chen,^a Yicheng Zhang,^b Siqi Chen,^b Qinhui Chen,^{b,c,*}

^a Department of Nursing, the First Affiliated Hospital of Fujian Medical University,
Fuzhou 350005, China

^b College of Chemistry and Materials Science, Fujian Normal University, Fuzhou
350007, People's Republic of China

^c Fujian Provincial Key Laboratory of Polymer Materials, Fujian Normal University,
Fuzhou 350007, People's Republic of China

† Electronic supplementary information (ESI) available

* Corresponding Author. E-mail addresses: chenqh@fjnu.edu.cn (Q. Chen)

Supporting information

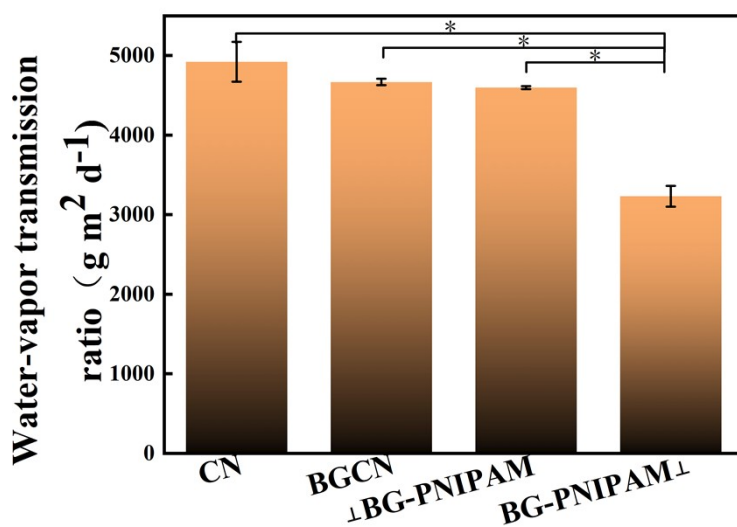


Figure S1 The water vapor transmission rate.

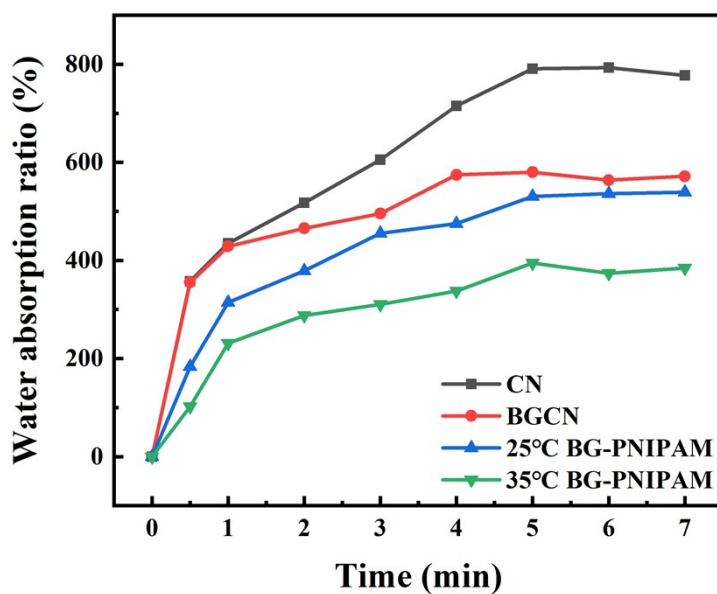


Figure S2 The water absorption ratio.

Movie S1 Infiltration of water from both sides of Janus gauze at different ambient temperatures.

Movie S2 Video of hemostasis in a rat liver injured model using BG-PNIPAM.

Movie S3 Video of hemostasis in a rat femoral artery injured model using BG-PNIPAM.